


Provides research grade measurements under all light sources, including LEDs

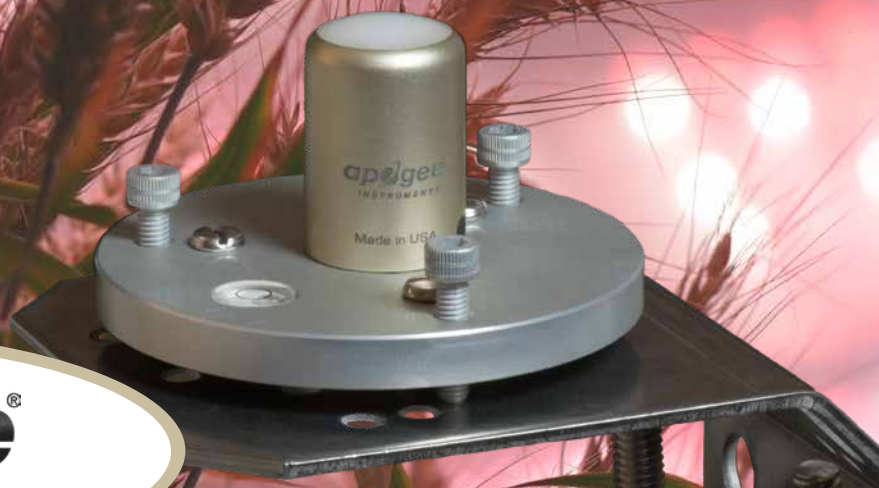

FULL-SPECTRUM QUANTUM SENSOR | SQ-521-SS & SQ-522-SS

Features

Accurate, Stable Measurements

Cosine-corrected with directional errors less than $\pm 5\%$ at a solar zenith angle of 75° . Long-term non-stability less than 2% per year.

Unique Design

Measure photosynthetically active radiation with a research grade, full spectral response sensor. The patented, dome-shaped aluminum head is cosine-corrected, self-cleaning, and fully-potted for a waterproof design.


No Datalogger Required

Connect sensor to a desktop, laptop, or tablet computer via a USB 2.0 type A plug. The ApogeeConnect software gives the user control of datalogging and calibration settings, provides real-time output display and graph of PPFD measurements, and allows the data set to be saved as a csv file for analysis. Sensor has internal data storage ability to hold up to 10,00 measurements.

Spectral Errors


	Apogee SQ-500	Apogee SQ-110 SQ-120	LI-COR LI-190	Kipp & Zonen
Sun (Clear Sky)	-2.2	0.0	-0.4	-1.0
Sun (Cloudy Sky)	-1.7	1.4	-0.2	-1.3
Sun (Reflected from Deciduous Leaves)	-2.0	4.9	-0.8	1.1
Sun (Transmitted below Wheat Canopy)	-1.1	6.4	-0.1	-0.3
Cool White Fluorescent (T5)	0.0	0.0	0.0	0.0
Metal Halide	0.9	-3.7	0.2	-1.7
Ceramic Metal Halide	-0.3	-6.0	0.4	-0.7
High Pressure Sodium	0.0	0.8	1.3	1.4
Red/Blue LED (16 % 444 nm, 84 % 667 nm peaks)	-3.4	-65.3	3.5	-1.8
Red/White LED (6.5 % 436 nm, 4.5 % 531 nm, 89 % 668 nm peaks)	-3.0	-60.3	2.6	-1.7

Cosine Response

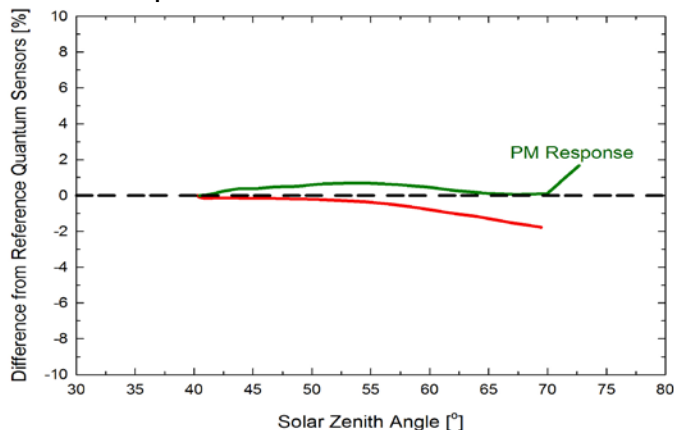

Mean cosine response of seven Apogee SQ-500 quantum sensors. Cosine response was calculated as the relative difference of SQ-500 quantum sensors from the mean of replicate reference quantum sensors (LI-COR models LI-190 and LI-190R, Kipp & Zonen model PQS 1). The red data are AM measurements; the green data are PM measurements.


Spectral Response

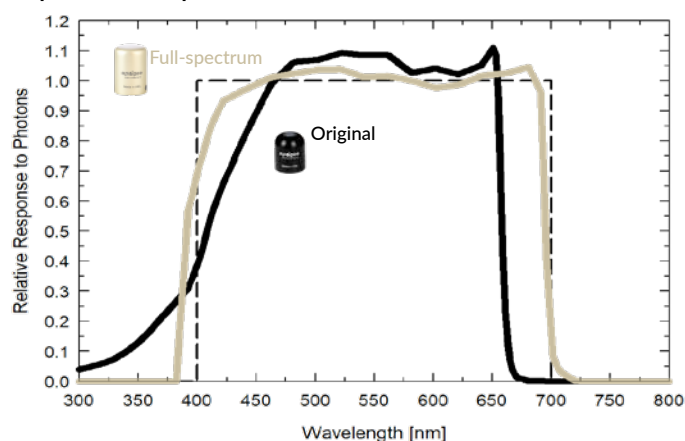

Mean spectral response measurements of six replicate Apogee SQ-100 and SQ-500 series quantum sensors. Spectral response measurements were made at 10 nm increments across a wavelength range of 300 to 800 nm in a monochromator with an attached electric light source. Measured spectral data from each quantum sensor were normalized by the measured spectral response of the monochromator/electric light combination, which was measured with a spectroradiometer.

Calibration Traceability

Apogee SQ-500 sensors are calibrated through side-by-side comparison to the mean of four transfer standard sensors under a reference lamp. The reference sensors are recalibrated with a quartz halogen lamp traceable to the National Institute of Standards and Technology (NIST).

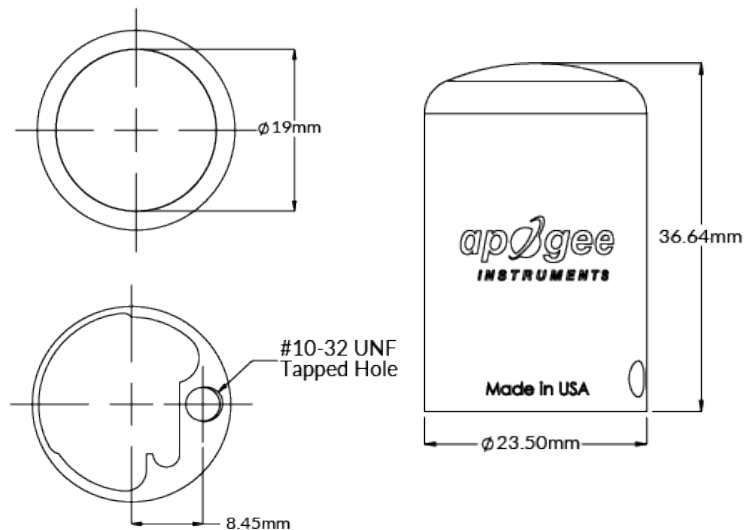

Product Specifications

SQ-520	
Power Supply	Uses a 5 V USB power source; 2.1 mA current draw when logging
Resolution	$0.1 \mu\text{mol m}^{-2} \text{s}^{-1}$
Calibration Factor	Custom for each sensor and stored in the firmware
Calibration Uncertainty	$\pm 5 \%$
Measurement Repeatability	Less than 0.5 %
Long-term Drift (non-stability)	Less than 2 % per year
Non-linearity	Less than 1 % (up to $4000 \mu\text{mol m}^{-2} \text{s}^{-1}$)
Response Time	Software updates every second
Field of View	180°
Spectral Range	689 to 692 nm ± 5 nm (wavelengths where response is greater than 50 % of maximum)
Spectral Selectivity	Less than 10 % from 412 to 682 nm ± 5 nm
Directional (Cosine) Response	$\pm 5 \%$ at 75° zenith angle
Azimuth Error	Less than 0.5 %
Tilt Error	Less than 0.5 %
Temperature Response	$-0.11 \pm 0.03 \%$ per C
Uncertainty in Daily Total	Less than 5 %
Detector	Blue-enhanced silicon photodiode
Housing	Anodized aluminum body with acrylic diffuser
IP Rating	IP68
Operating Environment	-40 to 70 C; 0 to 100 % relative humidity; can be submerged in water up to depths of 30 m
Dimensions	24 mm diameter, 37 mm height
Mass	100 g (with 5 m of lead wire)
USB Cable	4.6 m (15 ft)
Warranty	4 years against defects in materials and workmanship